
COCIR
Advancing Healthcare

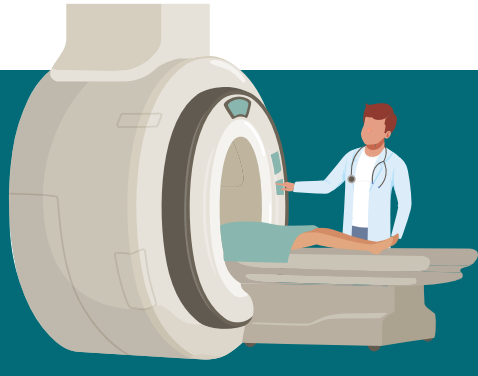

AGE PROFILE & DENSITY


MEDICAL IMAGING EQUIPMENT

2026 EDITION

MOLECULAR IMAGING POSITRON EMISSION TOMOGRAPHY (MI-PET/CT)


MI-PET/CT **AGE PROFILE**

THE COCIR GOLDEN RULES




1. 60% At least **60%** of the installed equipment base should be **less than five years old**.
2. 30% No more than **30%** of the installed equipment base should be **between six to ten years old**.
3. 10% No more than **10%** of the age profile should be **more than ten years old**.

APPROPRIATE MIX IN THE AGE PROFILE OF INSTALLED EQUIPMENT

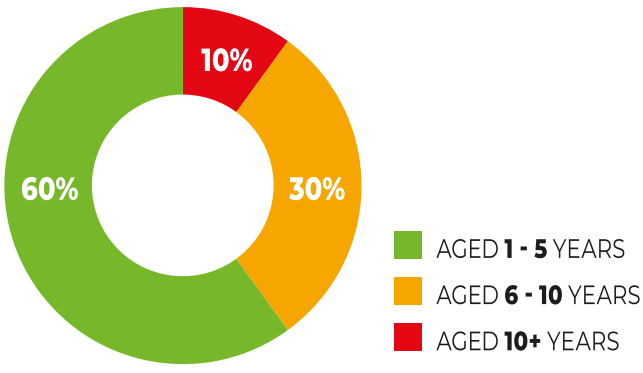

MI-PET/CT UNITS / COMPLIANCE WITH GOLDEN RULES / **EUROPE**

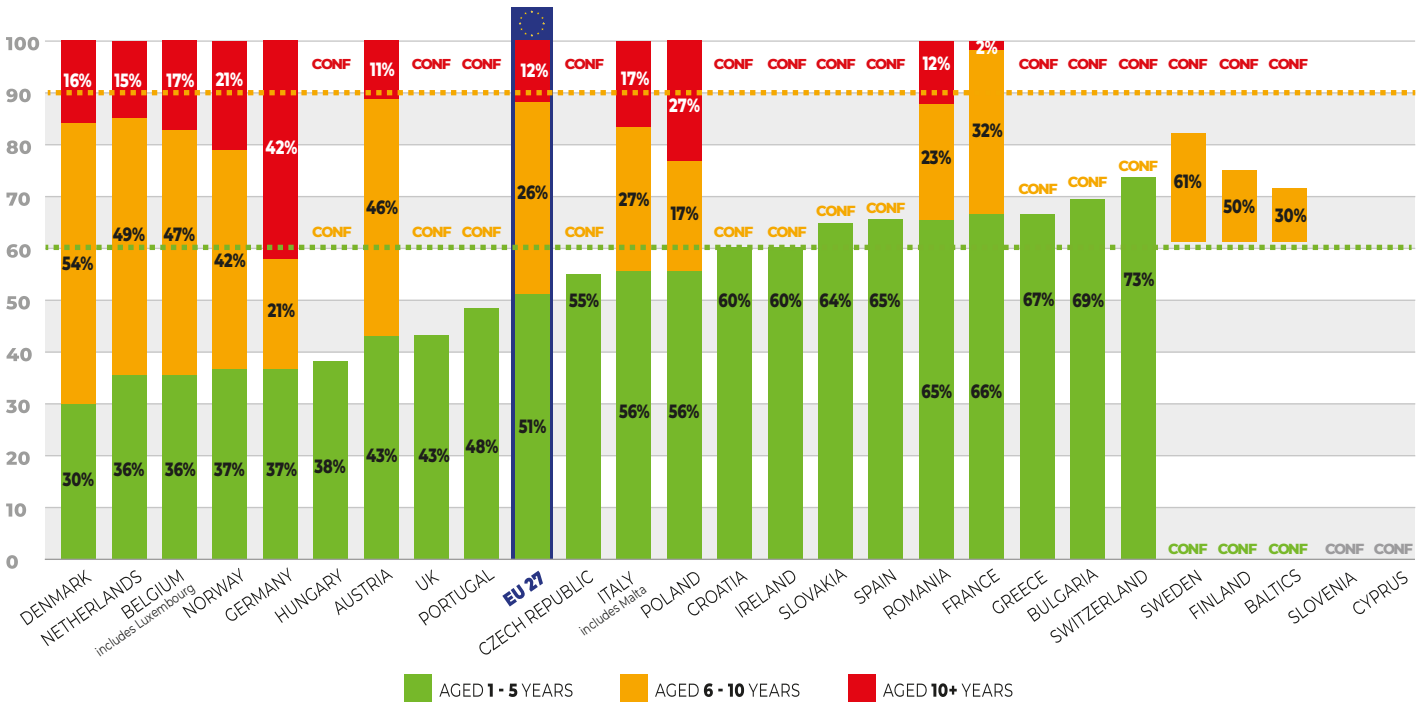

1/5

Approximately **one fifth** of the MI-PET/CT installed base in Europe is now **MORE THAN 10 YEARS OLD**




The majority of these MI-PET/CT units are in: **GERMANY**, **ITALY**, **THE NETHERLANDS** and **POLAND.**



MI-PET/CT **DENSITY**

MI-PET/CT UNITS / MILLION INHABITANTS / **EUROPE**

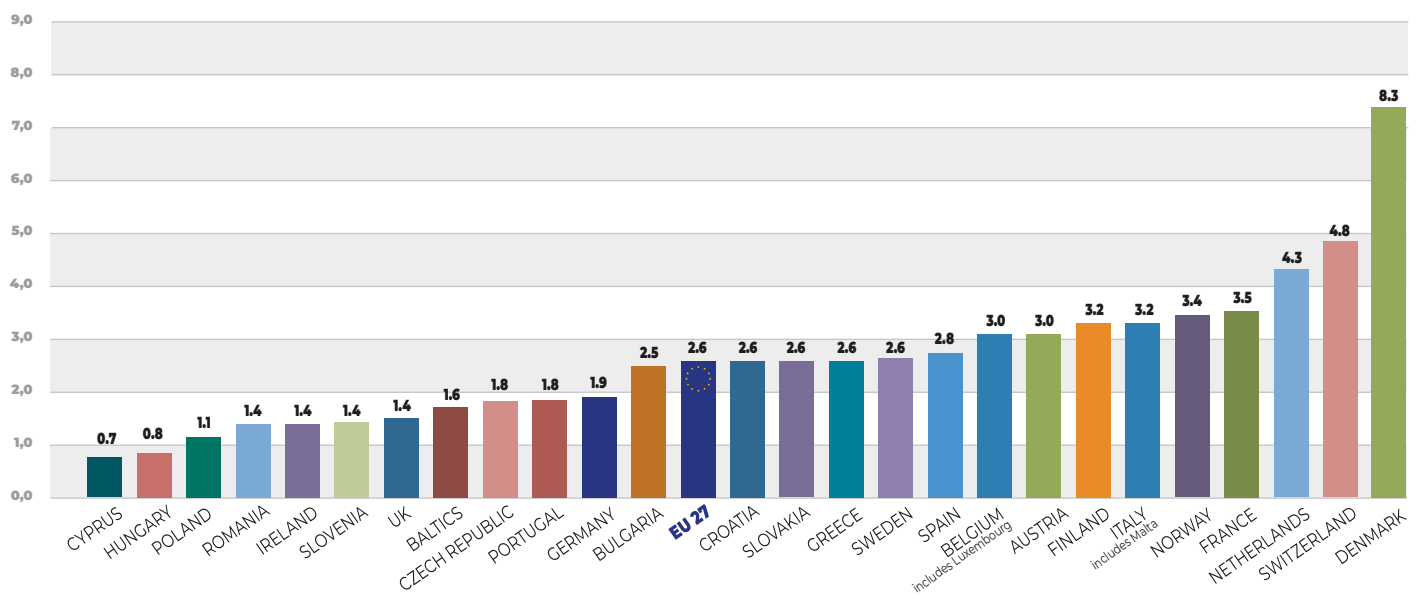

The data as per 31 December 2025, has been provided by the following COCIR member Companies:

Canon Medical Systems; **GE HealthCare**; **Philips Healthcare**; **Siemens Healthineers.**

Some data is CONF (Confidential) in compliance with EU Competition Law.