


AGE PROFILE & DENSITY MEDICAL IMAGING EQUIPMENT 2026 EDITION X-RAY MAMMOGRAPHY




X-RAY MAMMOGRAPHY AGE PROFILE

THE COCIR GOLDEN RULES

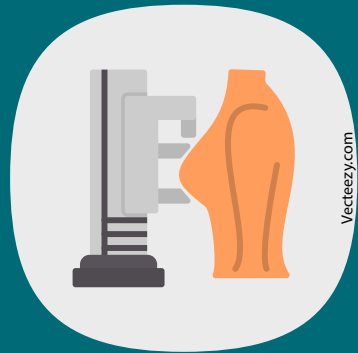


- 60%** At least **60%** of the installed equipment base should be **less than five years old**.
- 30%** No more than **30%** of the installed equipment base should be **between six to ten years old**.
- 10%** No more than **10%** of the age profile should be **more than ten years old**.

APPROPRIATE MIX IN THE AGE PROFILE OF INSTALLED EQUIPMENT

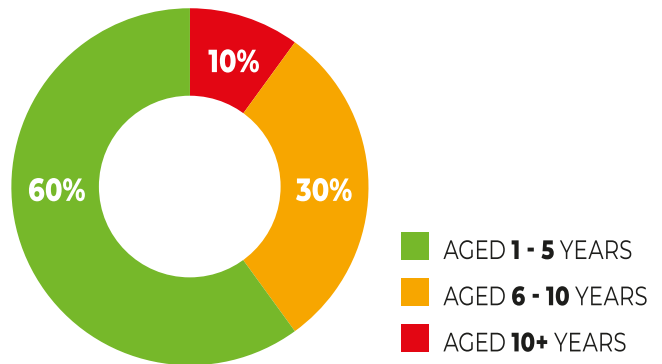


X-RAY MAMMOGRAPHY UNITS / COMPLIANCE WITH GOLDEN RULES / EUROPE

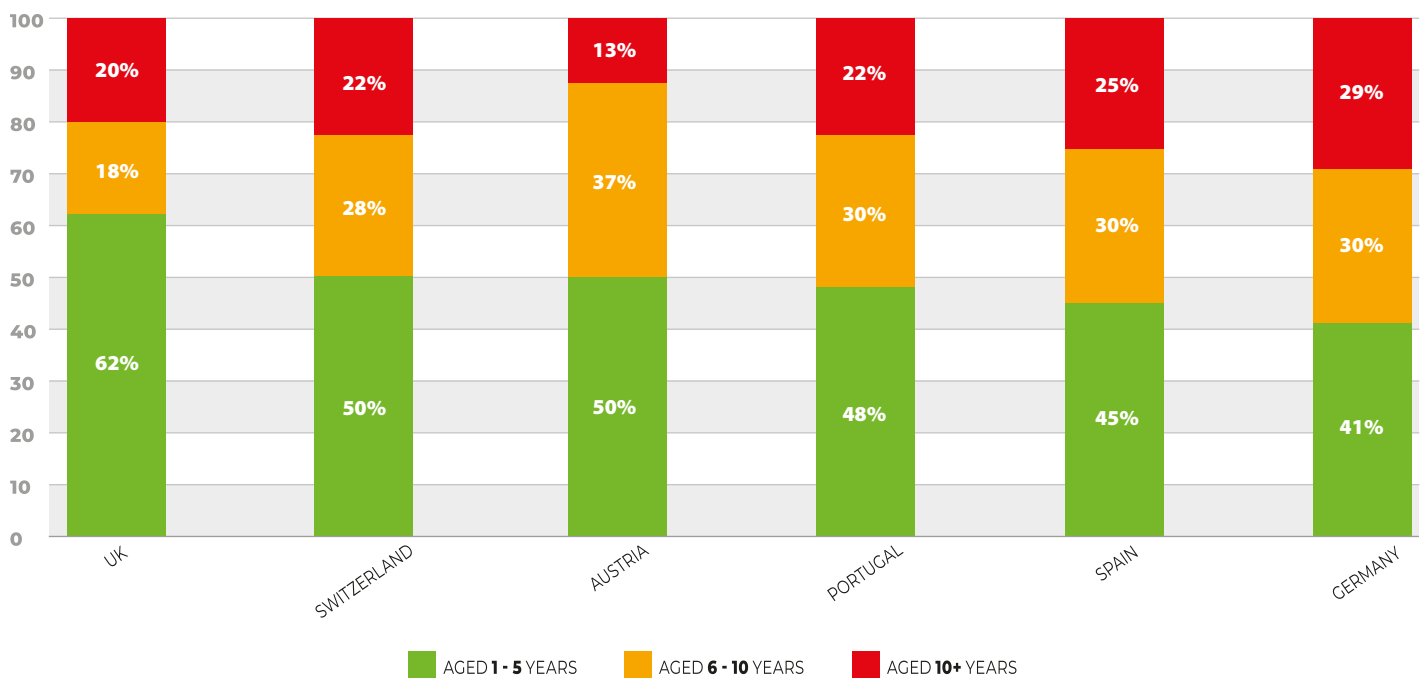


1/4

Approximately **one fourth** of the X-Ray Mammography installed base in the European countries analysed is now **MORE THAN 10 YEARS OLD**

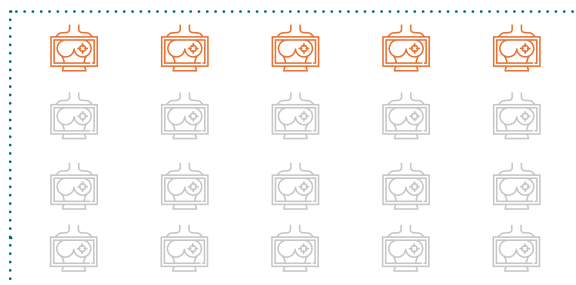

X-RAY MAMMOGRAPHY DENSITY

X-RAY MAMMOGRAPHY UNITS / MILLION INHABITANTS / EUROPE

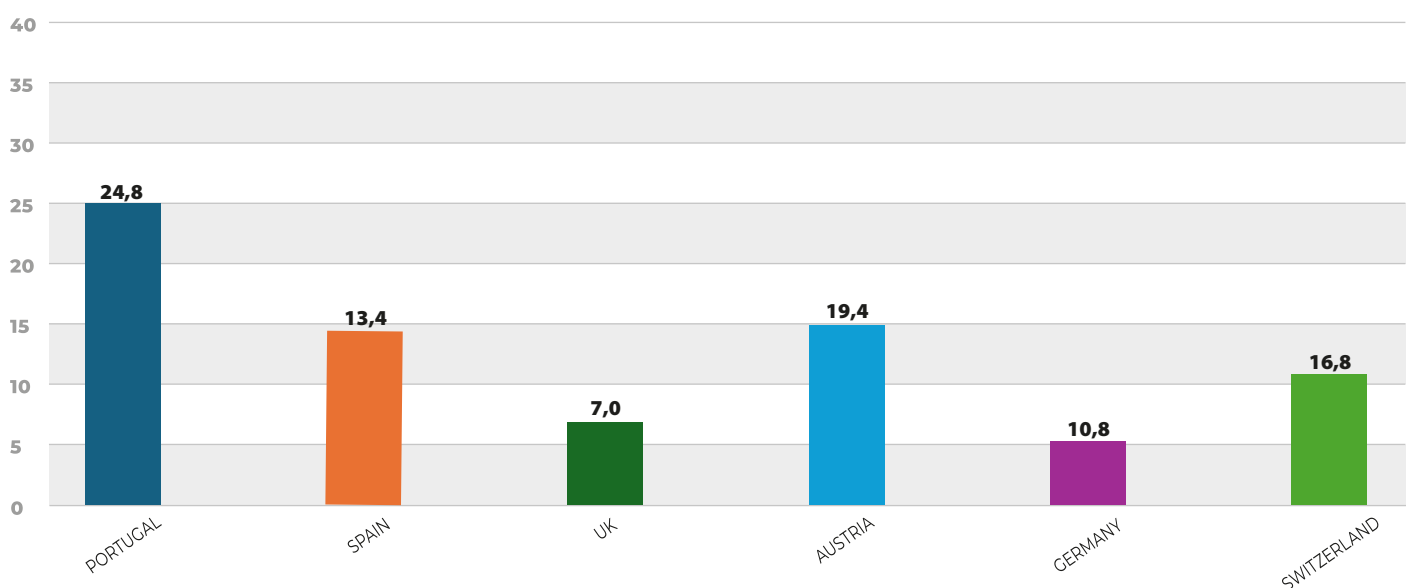

The data as per 31 December 2025, has been provided by the following COCIR member Companies:
Canon Medical Systems; Fujifilm; GE HealthCare; Philips Healthcare; Siemens Healthineers